Certificate of Analysis

ANALYZED BY:
Anresco Laboratories
1375 Van Dyke Avenue,
San Francisco, CA 94124
C8-0000052-LIC

CUSTOMER:
Kiva Products, LLC
2300 N Loop Rd
Alameda 94502
n/a

MANUFACTURER:
Atlantic Candy Company
St Augustine
St Augustine 32086



SAMPLE INFORMATION

Sample No.: 1391424
Product Name: Kiva Camino Sours Hemp Tropical Burst
Matrix: Edible (Gummy)
Lot #: KV22260310-53722

Date Collected: 03/12/2026
Date Received: 03/13/2026
Date Reported: 03/20/2026

TEST SUMMARY

Cannabinoid Profile:	Tested	**Microbiological Screen:**	Pass
Pesticide Residue Screen:	Pass	**Residual Solvent Screen:**	Pass
Heavy Metal Screen:	Pass	**Mycotoxin Screen:**	Pass
Water Activity:	Pass		

Cannabinoid Profile Tested

03/13/2026

Method: MF-CHEM-15
Instrument: Liquid Chromatography Diode Array Detector (LC-DAD)
Limit of Detection 0.0333 mg/g
Limit of Quantitation 0.1000 mg/g
Measurement of Uncertainty Average: ±6.3%

Cannabinoid	mg/g	%	mg/serving
Δ8-THC	ND	ND	ND
Δ9-THC	2.52	0.252	9.84
Δ9-THCA	ND	ND	ND
THCV	1.29	0.129	5.02
THCVA	ND	ND	ND
CBD	ND	ND	ND
CBDA	ND	ND	ND
CBC	ND	ND	ND
CBCA	ND	ND	ND
CBDV	ND	ND	ND
CBG	<LOQ	<LOQ	<LOQ
CBGA	ND	ND	ND
CBN	ND	ND	ND
Exo-THC	ND	ND	ND
(6aR,9R)-Δ10-THC	ND	ND	ND
(6aR,9S)-Δ10-THC	ND	ND	ND
9(R)-Hexahydrocannabinol	ND	ND	ND
9(S)-Hexahydrocannabinol	ND	ND	ND
Δ8-THC-O-Acetate	ND	ND	ND
Δ9-THC-O-Acetate	ND	ND	ND
THC-O-Phosphate	NT	NT	NT
δ8-THCP	ND	ND	ND
δ9-THCP	ND	ND	ND
Total THC	2.52	0.252	9.84
Total CBD	ND	ND	ND
Total Cannabinoids	3.81	0.381	14.86
Sum of Cannabinoids	3.81	0.381	14.86
Serving Weight (g)	3.9		

Total THC = Δ8-THC + Δ9-THC + (0.877 * THCA)
Total CBD = CBD + (0.877 * CBDA)
Total Cannabinoids = Σ (neutral cannabinoids) + [0.877 * Σ (acidic cannabinoids)]

This document is intended only for the use of the party to whom it is addressed and may contain information that is privileged, confidential or protected from disclosure under applicable law. Sampling was not performed by the laboratory. Results apply only to the sample(s) as received.

Microbiological Screen ✔ Pass

03/19/2026

Measurement of Uncertainty Average: APC ±35.6%, Y&M ±31.3%

Analyte	Findings	Units	Method	Limit	Status
Salmonella	ND	/10g	AOAC 2016.01	ND	Pass
STEC	ND	/10g	MF-MICRO-18	ND	Pass
Aspergillus flavus	ND	/10g	MF-MICRO-14	ND	Pass
Aspergillus fumigatus	ND	/10g	MF-MICRO-14	ND	Pass
Aspergillus niger	ND	/10g	MF-MICRO-14	ND	Pass
Aspergillus terreus	ND	/10g	MF-MICRO-14	ND	Pass
Listeria Species	ND	/10g	AOAC 2016.07	ND	Pass
Total Aerobic Plate Count	<10	cfu/g	FDA BAM	100000	Pass
Total Coliforms	<10	cfu/g	FDA BAM - ECC Agar	100	Pass
E. Coli	ND	/1g	FDA BAM Modified	1	Pass
Total Enterobacteriaceae	<10	cfu/g	AOAC 2003.01	ND	Pass
Staphylococcus aureus	<10	cfu/g	AOAC 2003.07	ND	Pass
Total Yeast and Mold	<10	cfu/g	FDA BAM	100000	Pass

Pesticide Residue Screen ✔ Pass

03/19/2026

Method: MF-CHEM-13

Instrument: Liquid Chromatography Tandem Mass Spectrometry (LC-MS/MS) & Gas Chromatography Tandem Mass Spectrometry (GC-MS/MS)

Measurement of Uncertainty Average: ±21.40%

Analyte	LOD/LOQ (ppm)	Findings (ppm)	Limit (ppm)	Status
Abamectin	0.015/0.05	ND	0.05	Pass
Acephate	0.003/0.01	ND	0.01	Pass
Acequinocyl	0.003/0.01	ND	0.01	Pass
Acetamiprid	0.003/0.01	ND	0.01	Pass
Aldicarb	0.003/0.01	ND	0.01	Pass
Azoxystrobin	0.003/0.01	ND	0.01	Pass
Bifenazate	0.003/0.01	ND	0.01	Pass
Bifenthrin	0.003/0.01	ND	0.01	Pass
Boscalid	0.003/0.01	ND	0.01	Pass
Captan	0.250/0.7	ND	0.7	Pass
Carbaryl	0.003/0.01	ND	0.01	Pass
Carbofuran	0.003/0.01	ND	0.01	Pass
Chlorantraniliprole	0.003/0.01	ND	0.01	Pass
Chlordane	0.020/0.06	ND	0.06	Pass
Chlorfenapyr	0.015/0.05	ND	0.05	Pass
Chlorpyrifos	0.003/0.01	ND	0.01	Pass
Clofentezine	0.003/0.01	ND	0.01	Pass
Coumaphos	0.003/0.01	ND	0.01	Pass
Cyfluthrin	0.015/0.05	ND	0.05	Pass
Cypermethrin	0.015/0.05	ND	0.05	Pass
Daminozide	0.003/0.01	ND	0.01	Pass
DDVP (Dichlorvos)	0.003/0.01	ND	0.01	Pass
Diazinon	0.003/0.01	ND	0.01	Pass
Dimethoate	0.003/0.01	ND	0.01	Pass
Dimethomorph	0.003/0.01	ND	0.01	Pass
Ethoprop(hos)	0.003/0.01	ND	0.01	Pass
Etofenprox	0.003/0.01	ND	0.01	Pass
Etoxazole	0.003/0.01	ND	0.01	Pass
Fenhexamid	0.007/0.02	ND	0.02	Pass
Fenoxycarb	0.003/0.01	ND	0.01	Pass
Fenpyroximate	0.007/0.02	ND	0.02	Pass
Fipronil	0.003/0.01	ND	0.01	Pass
Flonicamid	0.003/0.01	ND	0.01	Pass
Fludioxonil	0.003/0.01	ND	0.01	Pass
Hexythiazox	0.003/0.01	ND	0.01	Pass
Imazalil	0.003/0.01	ND	0.01	Pass
Imidacloprid	0.003/0.01	ND	0.01	Pass
Kresoxim Methyl	0.003/0.01	ND	0.01	Pass
Malathion	0.003/0.01	ND	0.01	Pass
Metalaxyl	0.003/0.01	ND	0.01	Pass
Methiocarb	0.003/0.01	ND	0.01	Pass
Methomyl	0.003/0.01	ND	0.01	Pass
Methyl parathion	0.003/0.01	ND	0.01	Pass
Mevinphos	0.007/0.02	ND	0.02	Pass

This document is intended only for the use of the party to whom it is addressed and may contain information that is privileged, confidential or protected from disclosure under applicable law. Sampling was not performed by the laboratory. Results apply only to the sample(s) as received.

Analyte	LOD/LOQ (ppm)	Findings (ppm)	Limit (ppm)	Status
Myclobutanil	0.003/0.01	ND	0.01	Pass
Naled	0.003/0.01	ND	0.01	Pass
Oxamyl	0.003/0.01	ND	0.01	Pass
Paclobutrazol	0.003/0.01	ND	0.01	Pass
Pentachloronitrobenzene	0.003/0.01	ND	0.01	Pass
Permethrins	0.015/0.05	ND	0.05	Pass
Phosmet	0.003/0.01	ND	0.01	Pass
Piperonyl Butoxide	0.003/0.01	ND	0.01	Pass
Prallethrin	0.015/0.05	ND	0.05	Pass
Propiconazole	0.003/0.01	ND	0.01	Pass
Propoxur	0.003/0.01	ND	0.01	Pass
Pyrethrins	0.015/0.05	ND	0.05	Pass
Pyridaben	0.003/0.01	ND	0.01	Pass
Spinetoram	0.003/0.01	ND	0.01	Pass
Spinosad	0.003/0.01	ND	0.01	Pass
Spiromesifen	0.003/0.01	ND	0.01	Pass
Spirotetramat	0.003/0.01	ND	0.01	Pass
Spiroxamine	0.003/0.01	ND	0.01	Pass
Tebuconazole	0.003/0.01	ND	0.01	Pass
Thiacloprid	0.003/0.01	ND	0.01	Pass
Thiamethoxam	0.003/0.01	ND	0.01	Pass
Trifloxystrobin	0.003/0.01	ND	0.01	Pass
Azadirachtin	0.100/0.30	ND	0.3	Pass
Chlormequat Chloride	0.03/0.10	ND	0.1	Pass
MGK 264	0.03/0.10	ND	0.1	Pass

Residual Solvent Screen ✔ Pass

03/19/2026

Method: MF-CHEM-32

Measurement of Uncertainty Average: ±1.43%

Analyte	LOD/LOQ (µg/g)	Findings (µg/g)	Limit (µg/g)	Status
1,1-Dichloroethene	2/4	ND	8	Pass
1,2-Dichloroethane	0.2/0.5	ND	1	Pass
Acetone	14/40	ND	750	Pass
Acetonitrile	14/40	ND	60	Pass
Benzene	0.2/0.5	ND	1	Pass
n-Butane	14/40	ND	800	Pass
Chloroform	0.2/0.5	ND	1	Pass
Ethanol	14/40	226.00	5000	Pass
Ethyl acetate	14/40	ND	400	Pass
Ethyl ether	14/40	ND	500	Pass
Ethylene oxide	0.2/0.5	ND	1	Pass
n-Heptane	14/40	ND	500	Pass
n-Hexane	14/40	ND	100	Pass
Isopropyl alcohol	14/40	ND	500	Pass
Methanol	14/40	43.00	250	Pass
Methylene chloride	0.2/0.5	ND	1	Pass
n-Pentane	14/40	ND	750	Pass
Propane	14/40	ND	210	Pass
Toluene	14/40	ND	150	Pass
Total xylenes (ortho-, meta-, para-)	14/40	ND	150	Pass
Trichloroethylene	0.2/0.5	ND	1	Pass

Heavy Metal Screen ✔ Pass

03/20/2026

Method: MF-CHEM-16

Instrument: Inductively Coupled Plasma Mass Spectrometry (ICP-MS)

Measurement of Uncertainty Average: ±4.4%

Analyte	LOD / LOQ (µg/g)	Findings (µg/g)	Limit	Status
Arsenic	0.033/0.101	ND	0.2	Pass
Cadmium	0.047/0.141	ND	0.2	Pass
Mercury	0.014/0.05	ND	0.1	Pass
Lead	0.107/0.324	ND	0.5	Pass

This document is intended only for the use of the party to whom it is addressed and may contain information that is privileged, confidential or protected from disclosure under applicable law. Sampling was not performed by the laboratory. Results apply only to the sample(s) as received.

Mycotoxin Screen ✔ Pass

03/19/2026

Method: MF-CHEM-13

Instrument: Liquid Chromatography Tandem Mass Spectrometry (LC-MS/MS) & Gas Chromatography Tandem Mass Spectrometry (GC-MS/MS)

Measurement of Uncertainty (MU): ±20.21%

Analyte	LOD/LOQ (ppb)	Findings (ppb)	Limit (ppb)	Status
Aflatoxin B1	2/5	ND	5	Pass
Aflatoxin B2	2/5	ND	20	Pass
Aflatoxin G1	2/5	ND	20	Pass
Aflatoxin G2	2/5	ND	20	Pass
Total Aflatoxins	8/20	ND	20	Pass
Ochratoxin A	2/5	ND	5	Pass

Water Activity ✔ Pass

03/19/2026


Method: MF-CHEM-14

Instrument: Water Activity Meter

Analyte	Findings (%)	Limit (%)	Status
Water Activity	0.70	0.85	Pass

ND = None Detected
LOD = Limit of Detection
LOQ = Limit of Quantitation

Reported by



Eric Tam
Senior Chemist

Scan to verify


This document is intended only for the use of the party to whom it is addressed and may contain information that is privileged, confidential or protected from disclosure under applicable law. Sampling was not performed by the laboratory. Results apply only to the sample(s) as received.

Cannabis Potency Report

<Sample Information>

Sample Name	: 1391424A 5x		
Sample ID	: run029		
Data Filename	: 1391424A 5x_run029_003.lcd		
Method Filename	: CanEX1_260220_CP5-14,-18.lcm		
Batch Filename	: 03-13-2026 processed.lcb		
Vial #	: 2-7	Sample Type	: Unknown
Injection Volume	: 5 uL		
Date Acquired	: 3/13/2026 4:40:48 PM	Acquired by	: System Administrator
Date Processed	: 3/13/2026 6:52:17 PM	Processed by	: System Administrator
Sample Amount	: 2.5471 grams		
Dilution Factor	: 250		

<Cannabinoid Chromatogram>

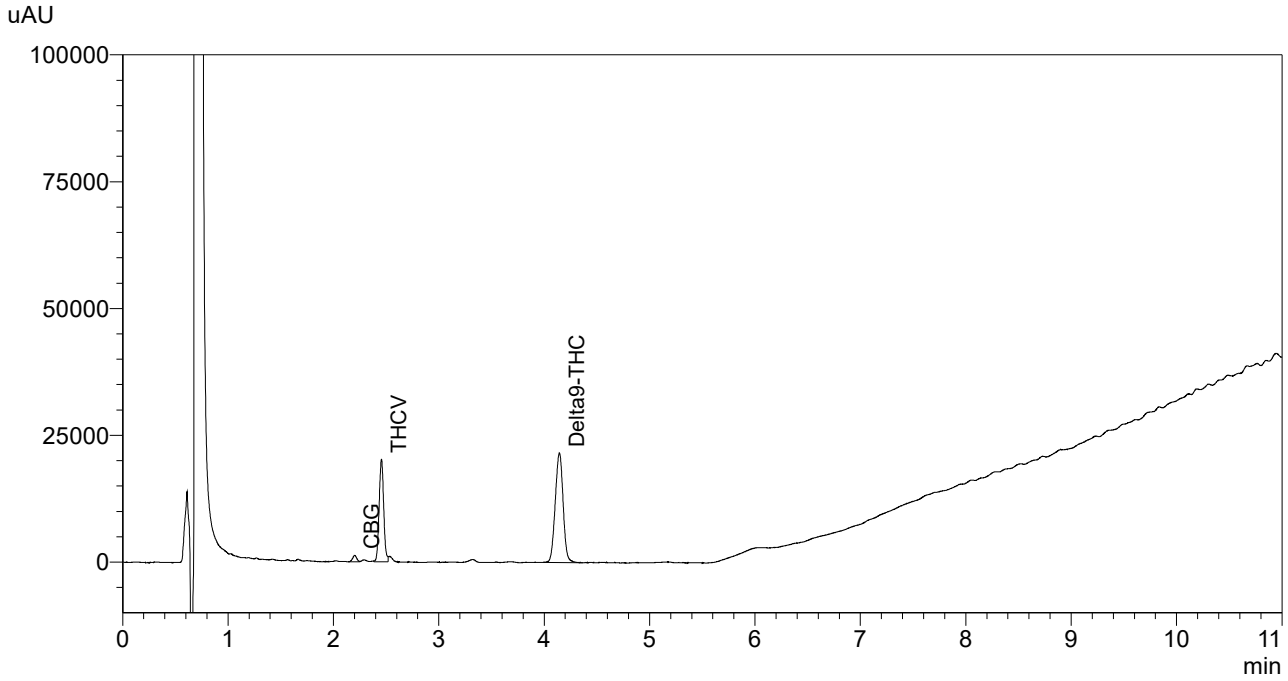

<Peak Table>

PDA Ch1 228nm


Peak#	Ret. Time	Name	Area	Height	Conc.	Unit
1	2.202	CBG	3448	1222	0.0623	mg/g
2	2.456	THCV	60908	19852	1.2749	mg/g
3	4.144	Delta9-THC	112211	21418	2.4914	mg/g

Cannabis Potency Report

<Sample Information>

Sample Name	: 1391424B 5x		
Sample ID	: run030		
Data Filename	: 1391424B 5x_run030_004.lcd		
Method Filename	: CanEX1_260220_CP5-14,-18.lcm		
Batch Filename	: 03-13-2026 processed.lcb		
Vial #	: 2-8	Sample Type	: Unknown
Injection Volume	: 5 uL		
Date Acquired	: 3/13/2026 4:54:10 PM	Acquired by	: System Administrator
Date Processed	: 3/13/2026 6:52:07 PM	Processed by	: System Administrator
Sample Amount	: 2.6324 grams		
Dilution Factor	: 250		

<Cannabinoid Chromatogram>

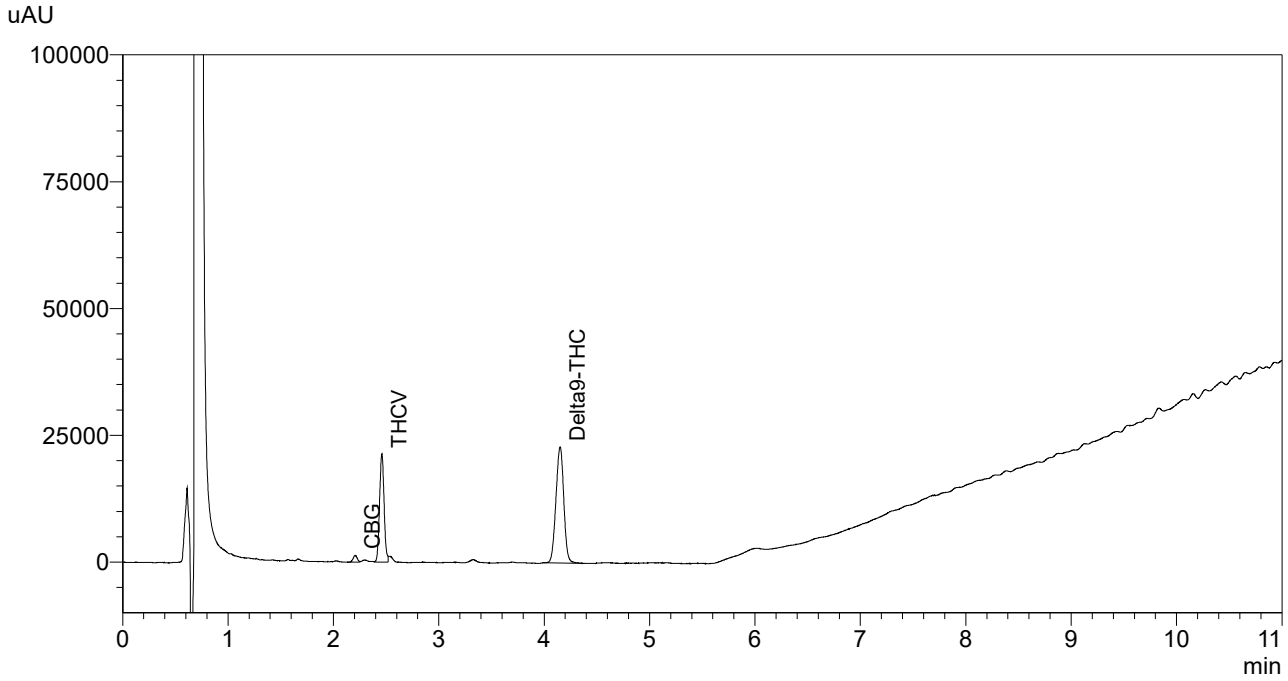

<Peak Table>

PDA Ch1 228nm

Peak#	Ret. Time	Name	Area	Height	Conc.	Unit
1	2.206	CBG	3726	1339	0.0659	mg/g
2	2.460	THCV	64100	21217	1.2988	mg/g
3	4.151	Delta9-THC	118896	22832	2.5545	mg/g